

# Comparison of in-vivo and ex-vivo Dielectric Properties of Biological Tissues

Saqib Salahuddin\*    Alessandra La Gioia\*    Muhammad Adnan Elahi\*  
Emily Porter\*    Martin O'Halloran\*    Atif Shahzad\*

*Abstract* —

Accurate knowledge of the dielectric properties of biological tissues are crucial for various applications such as assessment of specific absorption rate and safety of electromagnetic medical devices. Most of the available dielectric data in literature is based on *ex-vivo* measurements on biological tissue samples obtained from various animal models. This study investigates the differences in the *in-vivo* and *ex-vivo* dielectric properties of biological tissues, and variance over several animal species. The dielectric data is obtained from literature and organized to a unified format for comparison. The analysis shows considerable variations not only between *in-vivo* and *ex-vivo* dielectric properties of various tissues but also between various animal species.

## 1 INTRODUCTION

The dielectric properties of biological tissues have been widely studied at microwave and radio frequencies since the early 1950s [1–3]. These properties, namely, the conductivity and relative permittivity, determine the response of a material to an applied electromagnetic field [4]. The complex permittivity  $\varepsilon$  of a material is frequency dependent and is defined as:

$$\varepsilon(\omega) = \varepsilon'(\omega) - j\varepsilon''(\omega) \quad (1)$$

where  $j = \sqrt{-1}$ ,  $\omega$  is the angular frequency,  $\varepsilon'(\omega)$  is the relative permittivity (also called dielectric constant) and  $\varepsilon''(\omega)$  is the dielectric loss. The relative permittivity reflects the material's ability to store energy and the loss factor represents the energy dissipated in the material. The dielectric loss can be converted into effective conductivity using:

$$\sigma(\omega) = \omega\varepsilon_0\varepsilon''(\omega) \quad (2)$$

where  $\varepsilon_0$  is the permittivity of free space.

The precise knowledge of dielectric properties of biological tissues is essential for a wide variety of applications such as determination of Specific Absorption Rate (SAR) and evaluation of possible health hazards associated with non-ionising radiation, design and evaluation of electromagnetic diagnostic and therapeutic medical devices including microwave imaging and ablation [5–9].

\*Electrical and Electronic Engineering, National University of Ireland Galway, Ireland, e-mail: {S.salah-ud-din1, Martin.ohalloran, e.porter3}@nuigalway.ie, tel.: +353 91 524411.

A number of studies have reported *in-vivo* and *ex-vivo* dielectric properties of several biological tissues of human and animals over a wide frequency range of 10Hz to 40 GHz, using various measurement techniques. One of the largest and most comprehensive studies of the *ex-vivo* dielectric properties of human tissues was performed by Gabriel *et al.* over a wide frequency range of 10Hz to 20 GHz [10–12]. Other *ex-vivo* dielectric studies in past few decades for human and animal tissues includes [9, 13–19]. The literature on *in-vivo* dielectric properties of human and animal tissues includes [13, 14, 16, 20–23].

The available data in literature is in the form of either a graph, a table, or a mathematical parametric model that makes it difficult to collate and compare. In particular, there is limited data available in microwave frequency range and above. Such frequencies are important for potential medical applications and human safety concerns [6–8, 24]. Furthermore, there are conflicting views about the difference between the dielectric properties of *in-vivo* and *ex-vivo* tissues. Early studies suggest that there is a significant contrast between the *in-vivo* and *ex-vivo* dielectric properties of different biological tissues [9, 25]. The differences observed in relative permittivity were more prominent at lower frequencies, while the variation in conductivity values was high over the entire frequency spectrum. However, most recent studies have suggested that the contrast between *in-vivo* and *ex-vivo* dielectric properties is not significant provided that the environmental conditions and other physiological factors remain fixed [23, 26]. Recently, L. Farrugia *et al.* [23] performed *in-vivo* and *ex-vivo* dielectric measurements on rat liver tissue and concluded that temperature and dehydration are the major contributors to the difference between *ex-vivo* and *in-vivo* measurements. The uncertainty in the true dielectric properties of biological tissues can have a significant impact especially on microwave imaging and applications.

The purpose of this study is to: 1) collect and organize the available dielectric data on wide range of biological tissues from literature; 2) quantify the difference between in-vivo and ex-vivo dielec-

tric properties of different tissues; and 3) quantify the difference between dielectric properties of tissues from different species. In this study, the dielectric data only within microwave frequency range is considered, where most of the data is in range from 100 MHz to 40 GHz. It was not feasible to analyse the data for all the tissues in this paper. Therefore, four most widely studied tissues are selected from available data in literature for comparison.


## 2 Data Collection

The *in-vivo* and *ex-vivo* dielectric data of human and animal tissues was collected from literature over the frequency range of 100 MHz to 40 GHz. The temperature of the tissue samples in these studies varied from  $20^{\circ}C$  to  $38^{\circ}C$ . The dielectric data in literature is available in the form of graphs, tables, or dielectric models. To avoid any interpretation error, the data in graphical form was not included in the analysis. The data in tabular form was available for discrete frequencies and in some cases only one to two frequency points (915 MHz and 2.45 GHz). In contrast, dielectric models are valid for a wide frequency band, and dielectric properties can be inferred from these models for any frequency point within the band. In order to include maximum possible data, the comparison has been made against most common frequency points in the available data. The data was also translated to relative permittivity and conductivity expressed in  $S/m$  from various forms available in literature.


## 3 Results and Discussion

Fig. 1 (a) and (b) show *ex-vivo* and *in-vivo* dielectric properties of liver tissue for six different species, respectively. The data presented by solid lines was inferred from dielectric models while rest is the measured dielectric properties from different studies. Considering the diversity in available data, most common frequency point (915 MHz) is selected for comparison. It is also approved frequency for ablative therapy. The rectangular boxes in Fig. 1 highlight a significant variation in the available data. The overall variations in *ex-vivo* and *in-vivo* dielectric properties of tissues are 25.1% and %24.36, respectively. The variation in conductivity for both *ex-vivo* and *in-vivo* data is 35% and 25%.

Fig. 2 shows the comparison of *ex-vivo* and *in-vivo* dielectric properties of five different tissues at 915 MHz from bovine, ovine, porcine, rat, dog, cat and frog. Each box plot in the graph represents the dielectric properties of single tissue from different species. The single line in the figure represents that only one data sample is available. There is more

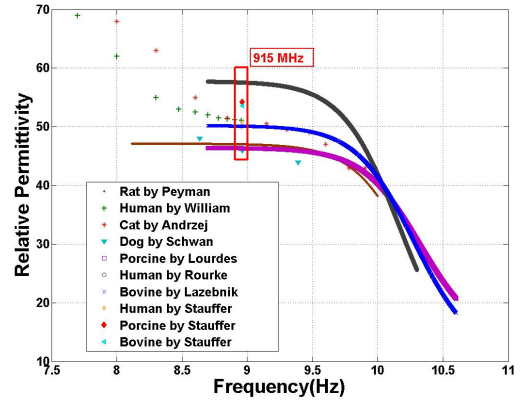

(a) Relative permittivity *ex-vivo* liver tissue

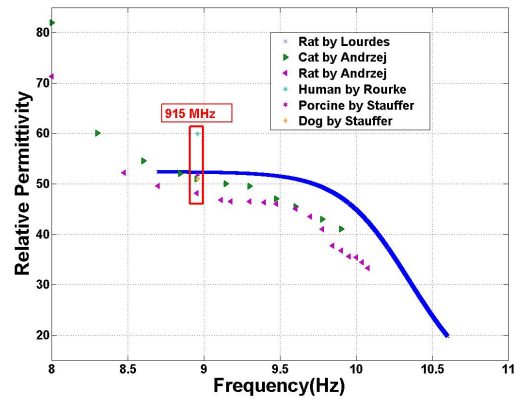


(b) Relative permittivity *in-vivo* liver tissue

Figure 1: Comparison of *ex-vivo* and *in-vivo* dielectric properties of liver tissue.


than 10% variation between species for all tissues especially for kidney, spleen and brain. There is a relatively large variation in conductivity, particularly in the case of spleen and kidney. The variation in all cases is more than the reported uncertainty of the measurement system, which can be either due to natural heterogeneity of tissue or inter-specie difference. Moreover, it is clear that even at single frequency point, the available data may not be representative of actual *in-vivo* dielectric properties of biological tissue.

## 4 Conclusion

In this study, the available dielectric data on wide range of biological tissues from literature was collected and organized. For analysis, the dielectric data within microwave frequency range was considered, where most of the data is in range from 100 MHz to 40 GHz. In this paper, a comparison of *in-vivo* and *ex-vivo* dielectric properties of

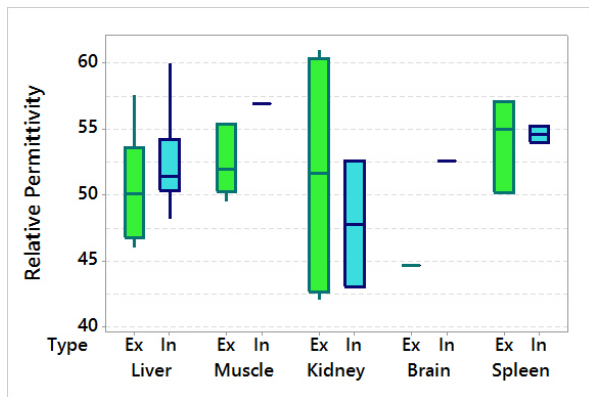

(a) Relative permittivity *ex-vivo* vs *in-vivo* for five different tissues

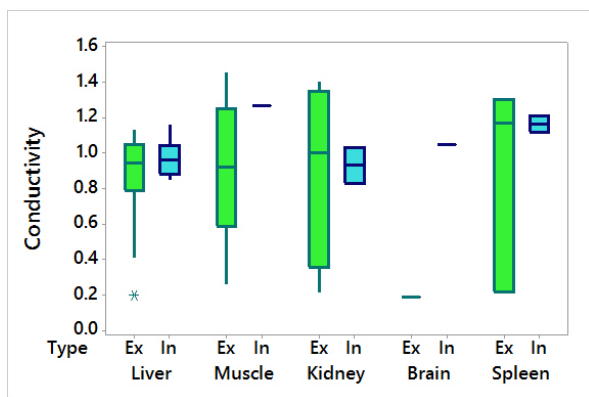

(b) Conductivity *ex-vivo* vs *in-vivo* for five different tissues

Figure 2: Inter-species comparison of *ex-vivo* and *in-vivo* dielectric properties of five different tissues at 915 MHz.

biological tissues has been presented. The results demonstrate a considerable variation up to 25% for permittivity and 30% for conductivity between *ex-vivo* and *in-vivo* dielectric properties of selected tissues. The results also demonstrate more than 25% variation between the dielectric properties of same tissue for different species. For microwave imaging and diagnostic device development, a slight error in the dielectric properties can have significant effect on the accuracy and reliability of the device. Moreover, the results suggest that the dielectric properties of tissues from an animal specie may not be applicable to other species, and a generalization of the data may not be valid. Further investigation is required to understand and characterize the variance between species.

### Acknowledgements

The research leading to these results has received funding from the European Research Council un-

der the ERC Grant Agreement n. 637780: 'BIO-ELECPRO' and Science Foundation Ireland Grant no. 15/ERC/S/3276. This work is also supported by the Irish Research Council (grant numbers RCS1325 and RCS1377) and has been developed in the framework of COST Action MiMed (TD1301).

### References

- [1] T. England, "Dielectric properties of the human body for wave-lengths in the 1–10 cm. range," *Nature*, vol. 166, no. 4220, pp. 480–481, 1950.
- [2] H. F. Cook, "The dielectric behaviour of some types of human tissues at microwave frequencies," *British Journal of Applied Physics*, vol. 2, no. 10, p. 295, 1951.
- [3] H. P. Schwan, "Electrical properties of tissue and cell suspensions," *Advances in biological and medical physics*, vol. 5, p. 147, 1957.
- [4] S. Salahuddin, E. Porter, F. Krewer, and M. O' Halloran, "Optimised analytical models of the dielectric properties of biological tissue," *Medical Engineering & Physics*, vol. 43, pp. 103–111, 2017.
- [5] ICNIRP, "Guidelines for limiting exposure to time-varying electric, magnetic, and electromagnetic fields (up to 300 GHz)," *Health Phys*, vol. 74, no. 4, pp. 494–522, 1998.
- [6] M. Persson, A. Fhager, H. Dob, Y. Yu, S. Member, T. Mckelvey, S. Member, J.-e. Karlsson, and M. Elam, "Microwave-Based Stroke Diagnosis Making Global Pre-hospital Thrombolytic Treatment Possible," *IEEE Transactions on Biomedical Engineering*, vol. 61, no. 11, pp. 2806–2817, 2014.
- [7] J. Bourqui, E. C. Fear, and J. M. Sill, "A Prototype System for Measuring Microwave Frequency Reflections from the Breast," *International Journal of Biomedical Imaging*, vol. 2012, pp. 1–12, jan 2012.
- [8] T. M. Grzegorzcyk, P. M. Meaney, P. A. Kaufman, R. M. Diflorio-Alexander, and K. D. Paulsen, "Fast 3-D tomographic microwave imaging for breast cancer detection," *IEEE Transactions on Medical Imaging*, vol. 31, no. 8, pp. 1584–1592, 2012.
- [9] R. J. Halter, T. Zhou, and P. M. Meaney, "The correlation of in vivo and ex vivo tissue dielectric properties to validate electromagnetic

- breast imaging: initial clinical experience,” *Physiological measurement*, vol. 30, no. 6, pp. 1–23, 2009.
- [10] C. Gabriel, S. Gabriel, and E. Corthout, “The dielectric properties of biological tissues: I. Literature survey.” *Physics in medicine and biology*, vol. 41, no. 11, pp. 2231–49, 1996.
- [11] S. Gabriel, C. Gabriel, and R. W. Lau, “The dielectric properties of biological tissues: II. Measurements in the frequency range 10 Hz to 20 GHz.” *Physics in medicine and biology*, vol. 41, no. 11, pp. 2251–2269, 1996.
- [12] C. Gabriel, “Compilation of the Dielectric Properties of Body Tissues at RF and Microwave Frequencies.” *Occupational and Environmental Health Directorate, Radiofrequency Radiation Division*, vol. Report No., no. June, pp. 1–23, 1996.
- [13] A. P. O’Rourke, M. Lazebnik, J. M. Bertram, M. C. Converse, S. C. Hagness, J. G. Webster, and D. M. Mahvi, “Dielectric properties of human normal, malignant and cirrhotic liver tissue: in vivo and ex vivo measurements from 0.5 to 20 GHz using a precision open-ended coaxial probe.” *Physics in medicine and biology*, vol. 52, no. 15, pp. 4707–19, 2007.
- [14] A. Kraszewski, M. A. Stuchly, S. S. Stuchly, and A. M. Smith, “In vivo and in vitro dielectric properties of animal tissues at radio frequencies.” *Bioelectromagnetics*, vol. 3, no. 4, pp. 421–432, 1982.
- [15] L. Chin and M. Sherar, “Changes in the dielectric properties of rat prostate ex vivo at 915 MHz during heating.” *International journal of hyperthermia : the official journal of European Society for Hyperthermic Oncology, North American Hyperthermia Group*, vol. 20, no. 5, pp. 517–527, 2004.
- [16] J. L. Schwartz and G. a. Mealing, “Dielectric properties of frog tissues in vivo and in vitro.” *Physics in medicine and biology*, vol. 30, no. 2, pp. 117–124, 1985.
- [17] R. D. Stoy, K. R. Foster, and H. P. Schwan, “Dielectric properties of mammalian tissues from 0.1 to 100 MHz: a summary of recent data.” *Physics in medicine and biology*, vol. 27, pp. 501–513, 1982.
- [18] A. Peyman, A. A. Rezazadeh, and C. Gabriel, “Changes in the dielectric properties of rat tissue as a,” *Group*, vol. 46, pp. 1617–1629, 2001.
- [19] L. Abdilla, C. Sammut, and L. Z. Mangion, “Dielectric properties of muscle and liver from 500 MHz–40 GHz,” *Electromagnetic Biology and Medicine*, vol. 32, no. 2, pp. 244–252, 2013.
- [20] M. a. Stuchly, A. Kraszewski, S. S. Stuchly, and a. M. Smith, “Dielectric properties of animal tissues in vivo at radio and microwave frequencies: comparison between species.” *Physics in medicine and biology*, vol. 27, no. 7, pp. 927–36, 1982.
- [21] P. R. Stauffer, F. Rossetto, M. Prakash, D. G. Neuman, and T. Lee, “Phantom and animal tissues for modelling the electrical properties of human liver,” *International Journal of Hyperthermia*, vol. 19, no. 910867416, pp. 89–101, 2003.
- [22] R. PETHIG, “Electrical Properties of Biological Tissue,” in *Electrical properties of tissue*, 2014, ch. 6, pp. 93–132.
- [23] L. Farrugia, P. S. Wismayer, L. Z. Mangion, and C. V. Sammut, “Accurate in vivo dielectric properties of liver from 500 MHz to 40 GHz and their correlation to ex vivo measurements,” *Electromagnetic Biology and Medicine*, vol. 8378, no. August, pp. 1–9, 2016.
- [24] J. Covington, R. Arasaradnam, and C. Nwokolo, “Diagnostic device. Patent US20130289368,” 2013.
- [25] K. R. Foster and H. Schwan, “Dielectric properties of tissues and biological materials: a critical review,” *Crit. Rev. Biomed. Eng.*, vol. 17, no. 1, pp. 25–104, 1989.
- [26] A. Peyman, S. Holden, and C. Gabriel, “Measurement of the Dielectric Properties of Biological Tissues in vivo at Microwave Frequencies,” Tech. Rep., 2009.